

# peca<sup>®</sup>



Forefoot  
Surgery

## Percutaneous Osteotomy Bunion implants Ø3 and Ø4 mm



**Exact-T<sup>®</sup> recess** - Precision  
**Beveled head** - Soft tissue preservation  
**Reduction wire** - Controlled metatarsal luxation


 **novastep<sup>®</sup>**  
Your foot & ankle company



PECA® Implant sytem provides a complete and versatile portfolio of **beveled fully threaded implants** intended for the fixation of osteotomy and arthrodesis of the foot.

The **Exact-T® Recess** provides **high precision** in fluoro percutaneous implant positioning. Specialized soft-tissue sparing burrs and percutaneous instrumentation are used in combination with the PECA® bunion implant system to perform bone cuts and provide stable fixation.



## PECA® Bunion implants

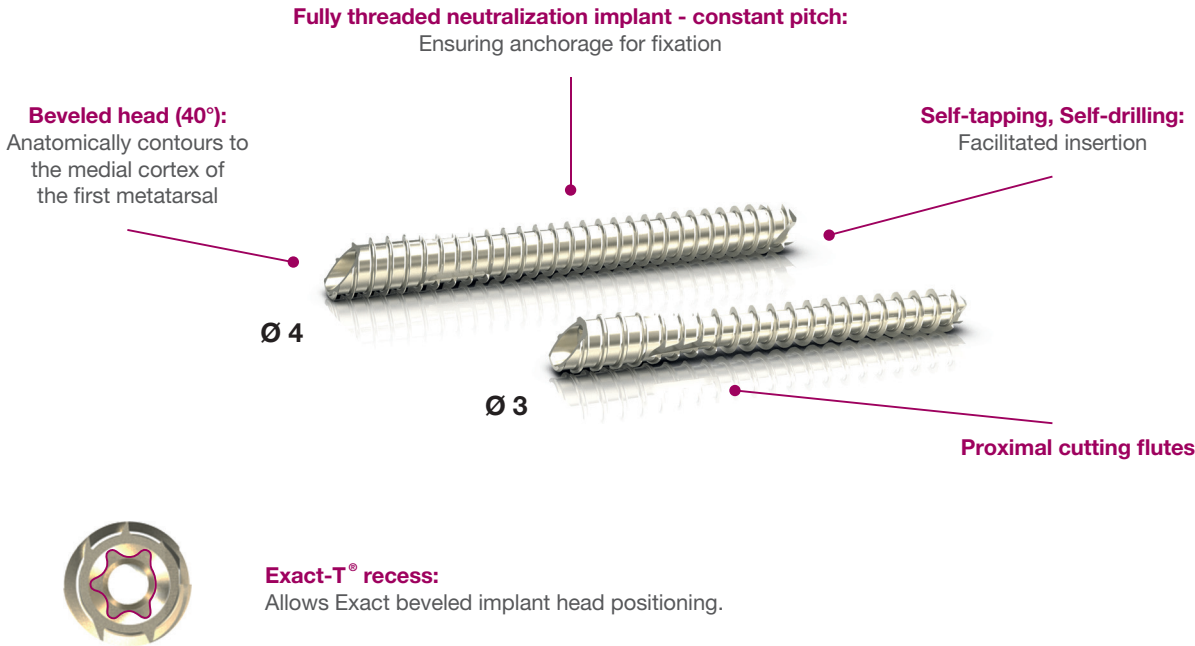

## PECA® Range


Made of Titanium alloy (TA6V Eli anodised), the PECA® Bunion implants is available in 3 mm and 4 mm diameters. Instrumentation is color-coded for convenient identification.

	<div>Ø3 PECA nexis</div> Ø 3 mm	<div>Ø4 PECA nexis</div> Ø 4 mm
Driver	Exact-T8	Exact-T10
Length	16 - 48 mm*	26 - 60 mm*
Guide-Wire	CoCr Ø 1.0 mm	CoCr Ø 1.4 mm
Drill Bits	Ø 2 mm	Ø 3.2 mm
	* 2 mm increments.	* 2 mm increments.

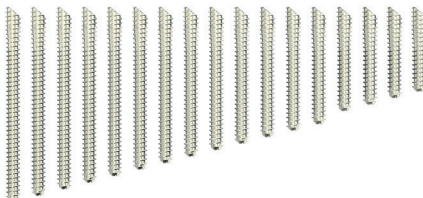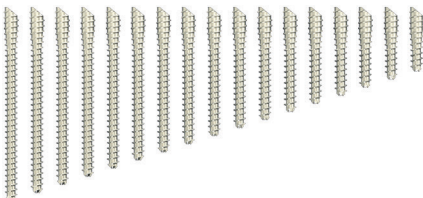



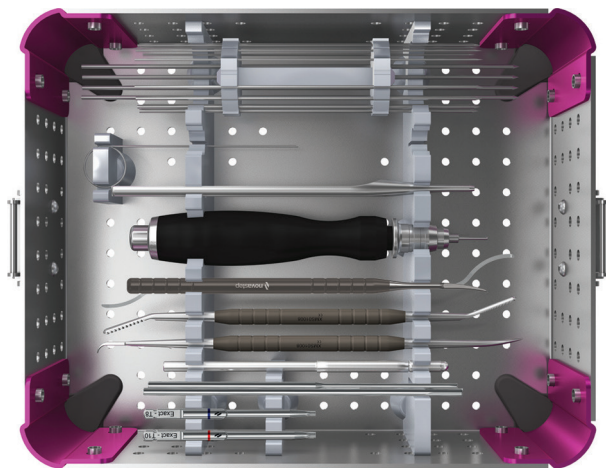


# PECA<sup>®</sup>, Specific and Percutaneous Instrumentation

The PECA<sup>®</sup> set combines **specific instrumentation** for PECA<sup>®</sup> implants and **percutaneous instrumentation** including periosteal elevator, rasps, reduction device, beaver blade holder dedicated percutaneous surgery.



## > Percutaneous Instruments:

-  Percutaneous rasp
-  Perioestal elevator double tip
-  Perioestal elevator single tip
-  *Reduction device double tip - Optional*
-  Beaver holder


## > Exact-T<sup>®</sup> Technology: patented innovation:

Exact-T<sup>®</sup> - Patent pending - facilitates correct placement of implant upon insertion.



## > Exact-T<sup>®</sup> recess:

**Specific:** easy indexing of the Exact-T<sup>®</sup> screwdriver tip. Allows exact driver positioning in **one direction only**.




## > Visual Guideline :

The black laser marking aligns with the beveled head of the implant, identifying the medial cortex of the first metatarsal, ensuring proper placement when implanted.

## > Sterile Percutaneous Burrs:

Intelligently designed single use burrs offer precision bone resection and removal without violating soft tissue structures.

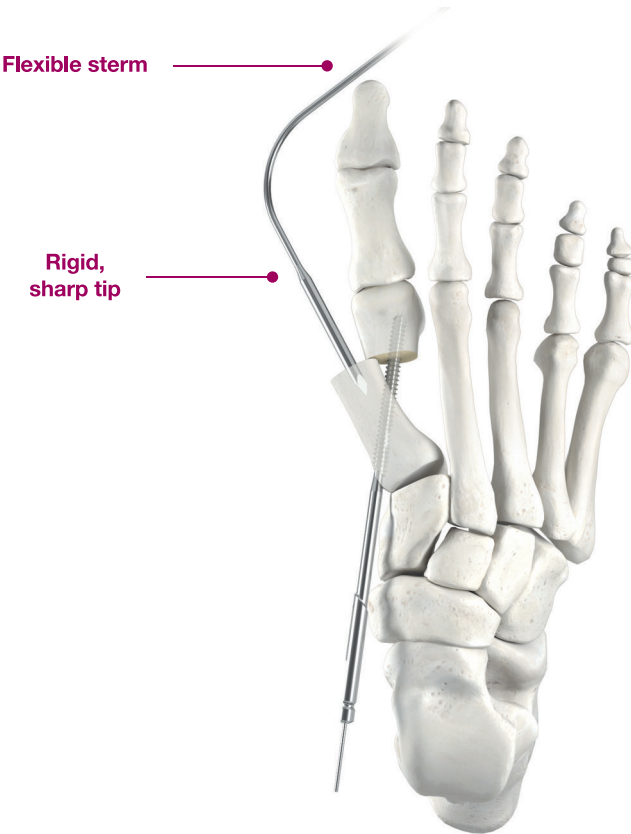

# References

## PECA® Bunion implants

Length (mm)	PECA® implant Ø 3 mm	PECA® implant Ø 4 mm
16 mm	PS020016	-
18 mm	PS020018	-
20 mm	PS020020	-
22 mm	PS020022	-
24 mm	PS020024	-
26 mm	PS020026	PS050026
28 mm	PS020028	PS050028
30 mm	PS020030	PS050030
32 mm	PS020032	PS050032
34 mm	PS020034	PS050034
36 mm	PS020036	PS050036
38 mm	PS020038	PS050038
40 mm	PS020040	PS050040
42 mm	PS020042	PS050042
44 mm	PS020044	PS050044
46 mm	PS020046	PS050046
48 mm	PS020048	PS050048
50 mm	-	PS050050
52 mm	-	PS050052
54 mm	-	PS050054
56 mm	-	PS050056
58 mm	-	PS050058
60 mm	-	PS050060

## K-wires, Reduction wire

Reference	Description
CKW02005	K-wire Ø 1.4 lg 150 mm TR/RD
CKW02004	K-wire Ø 1,0 lg 150 mm TR/RD
CKW03001	Reduction wire

## Indications




The osteosynthesis screws are indicated for arthrosis, hallux valgus and other bone alignment defaults (pes cavus, flatfoot, calcaneal valgus, malalignment secondary to previous trauma).

**Example of use:**  
Hallux Valgus with Percutaneous Chevron and Akin osteotomies.

# Sterile Percutaneous Burrs

Single use sterile burrs facilitate accurate bone resection and removal.

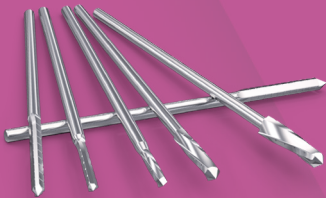

Reference	Description
CRE12008	Shannon Corta Ø 2 Lg 8 mm
CRE12012	Shannon Recta Ø 2 Lg 12 mm
CRE12222	Shannon Longa Ø 2.2 Lg 22 mm
CRE13020	Shannon Larga Ø 3 Lg 20 mm
CRE23113	Wedge 3.1 Lg 13 mm
CRE24113	Wedge 4.1 Lg 13 mm

 **Novastep:**  
2, Allée Jacques Frimot  
35000 RENNES - France  
Tel: + 33 (0) 2 99 33 86 50  
Fax: + 33 (0) 9 70 29 18 95  
contact@novastep-ortho.com  
www.int.novastep.life

**Please Note:**  
Carefully read the enclosed Instructions For Use (IFU) and all packaging label information.  
Devices: Implants: Class IIb-CE1639 / Instruments: Class I / Class IIa-CE1639.