



## Brochure

Pecaplasty® targeting guide




- . **Easy positioning** on the foot
- . **Controlled translation** of the metatarsal head
- . **Accurate placement** of the K-Wires


# pecaplasty®

Percutaneous Bunion Correction

The Pecaplasty® system allows for simple, precise and reproducible correction of Hallux Valgus in percutaneous surgery. With its easy positioning on the foot, the Pecaplasty® Targeting Guide allows controlled translation of the metatarsal head and accurate K-wires placement.

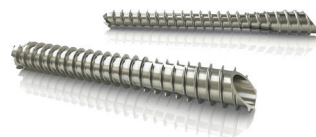



## Keys features

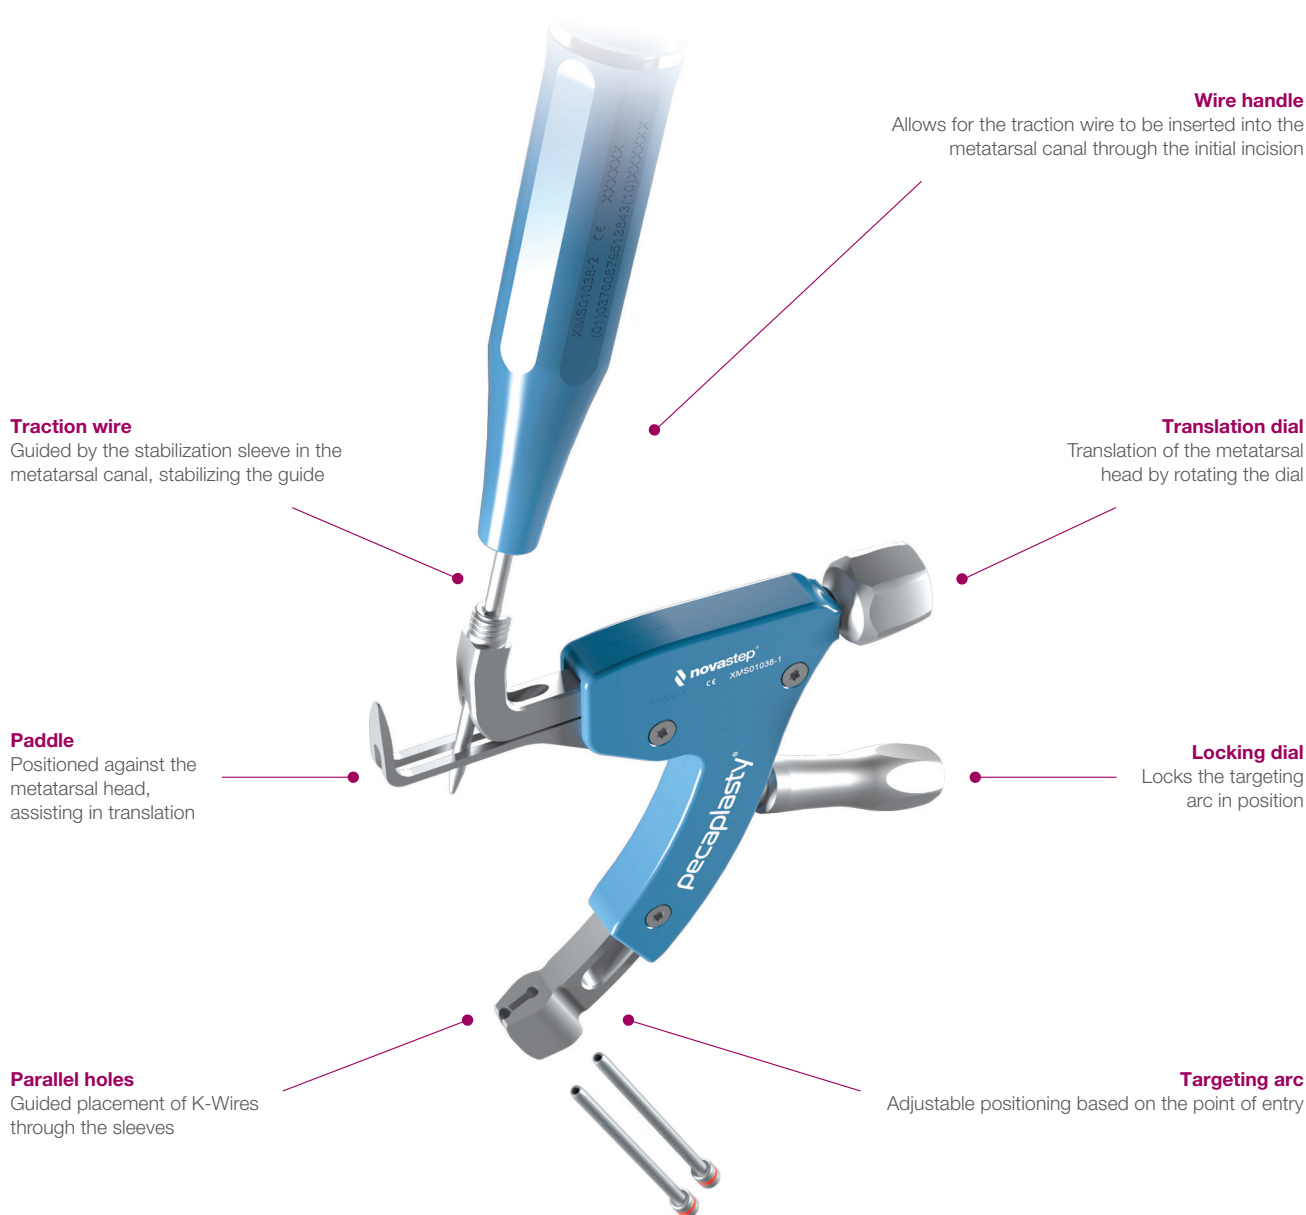

PATENT PENDING



# Guided & reproducible procedure

## 1 Easy positioning on the foot

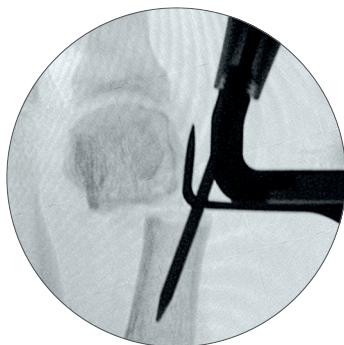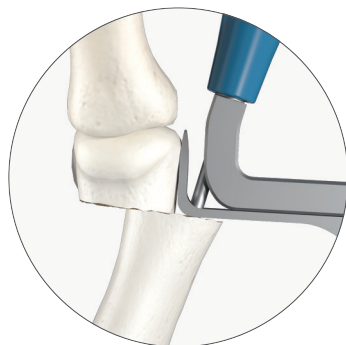



**POSITION** the guide by inserting the paddle underneath the medial capsule through initial incision, after a transverse osteotomy.

## 2 Controlled translation of metatarsal head

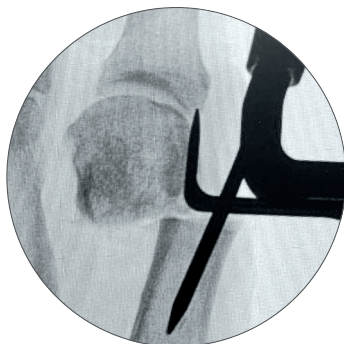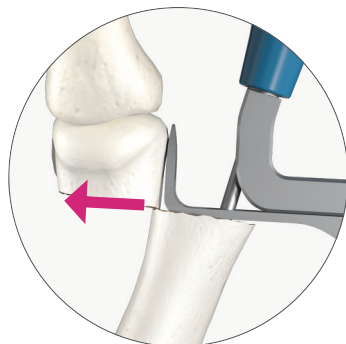

**TRANSLATE** the metatarsal head using the translation dial.


## 3 Accurate placement of K-Wires

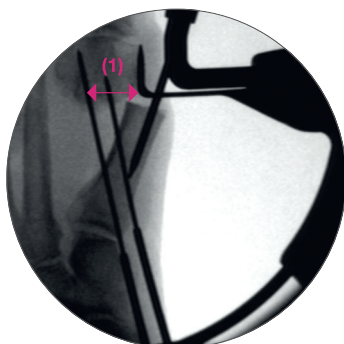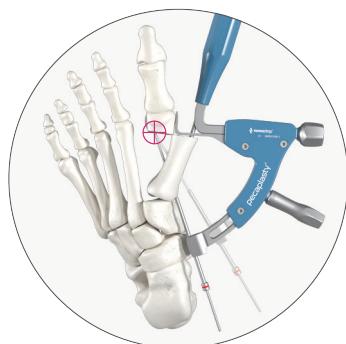

**ADJUST** the arc around its center of rotation to allow proper placement of the k-wires.

- Insertion point must be as proximal as possible to ensure bicortical fixation.
- Aiming point is fixed, always 14 mm (1) from the paddle.

Pecaplasty® targeting guide

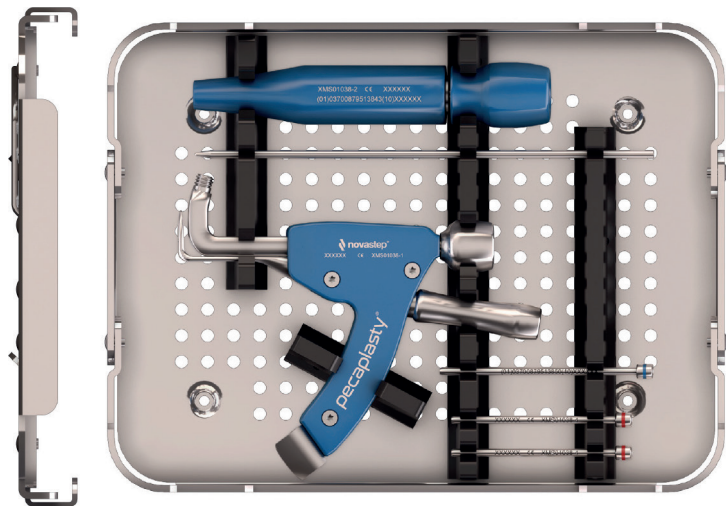

Reference	Designation	Qty	
XMS01038-1	Targeting guide	1	
XMS01038-2	Wire handle for targeting guide	1	
SKW06002*	Traction wire Ø 2.5 lg 128 - Sterile	5	
XMS01038-3	Peca® Ø 3 - K-wire sleeve for targeting guide	1	
XMS01038-4	Peca® Ø 4 - K-wire sleeve for targeting guide	2	

\*Non sterile traction wire is also available (Ref: CKW06002)

**Please Note:**  
Carefully read the enclosed Instructions For Use (IFU) and all packaging label information. Devices: Implants: Classe IIb-CE1639 / Instruments: Classe I / Classe IIa-CE1639.

**Novastep:**  
2, Allée Jacques Frimot - 35000 RENNES - France  
Tel: + 33 (0) 2 99 33 86 50 / Fax: + 33 (0) 9 70 29 18 95  
contact@novastep-ortho.com / www.int.novastep.life