



Brochure

—
Ø 4.0 PECA[®] Compressive

Beveled head canulated compressive implant



- . **Beveled head** - Optimum cortical anchorage
- . **Exact-T[®] recess** - Precision
- . **Dual partially threaded** - Optimal compression

Peca[®] Compressive Implants were designed to treat a wide range of forefoot and midfoot indications. The implant is equipped with a **beveled head** and partially threaded cutting flutes to maximize compression by seating flush with the near cortex, preserving soft tissue structures.

Keys features

Canulated implant titanium alloy TA6V ELI

Positive-Locking Channel:


As the implant is engaged into the bone the Positive Locking Channel pushes the excess bone toward the cortical surface increasing maximum compression and anchorage

Self-tapping & Self-Drilling:

Facilitate insertion

Beveled head (40°):


Dual partially threaded:
Optimal compression



Beveled head:

Cortical anchorage maximization and soft tissues preservation

VS



Standard head:


Compromise between burial of the head and cortical anchorage

Exact-T[®] recess:

Allows Exact beveled implant head positioning and provides optimal torque. The driver allows an exact positioning of the screwdriver tip in one position only.



Exact-T10 screwdriver

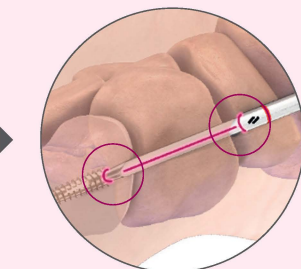

Visual guide



PECA[®] Compressive implants are available in Ø 4 mm and in lengths of 18 to 60 mm (with 2 mm increments up to 50 mm, then 5 mm increments).


Multiple indications

Peca® Compressive Implants can be used for the percutaneous fixation of fresh fractures and arthrodesis in the foot and ankle. Peca®-C can be used in combination with the Airlock® & Presslock® Plating Systems for procedures requiring the rigidity of a plate and screw construct.

Traditional surgery




Percutaneous surgery

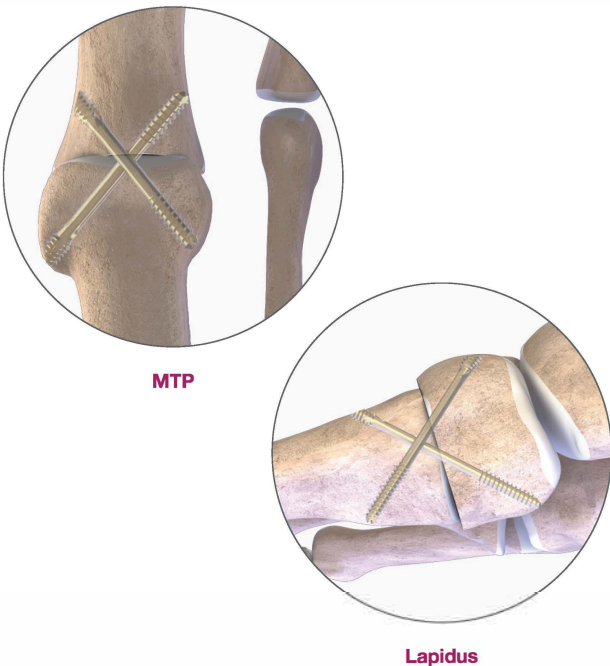

Dedicated instrumentation


- Ø 4.0 mm PECA® Compressive implant can be used:
- . With PECA® set, with the optional addition of a countersink;
 - . With AIRLOCK® set, with the addition of PECA® Compressive instruments.

PECA® Set

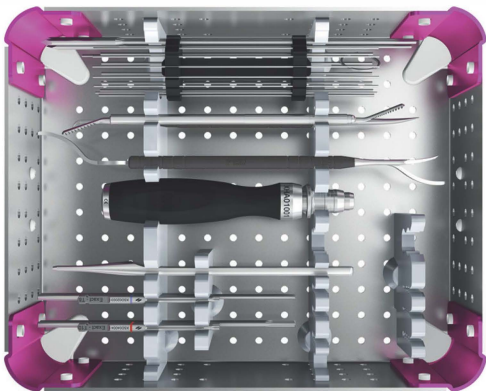

Countersink Ø 3.7 - optional

AIRLOCK® Set

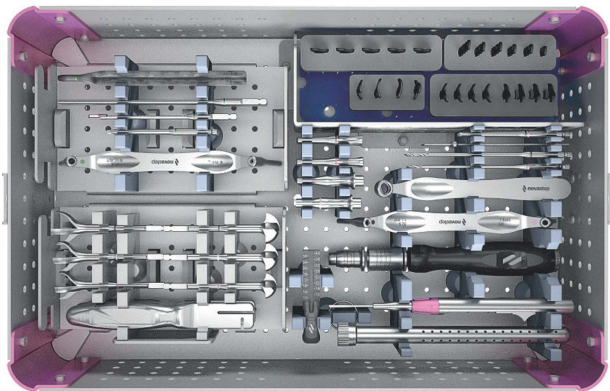

Exact-T®10 screwdriver tip



Drill bit Ø 3.2

References

PECA® Compressive implants



Length (mm)	Reference
18 mm	PS050118
20 mm	PS050120
22 mm	PS050122
24 mm	PS050124
26 mm	PS050126
28 mm	PS050128
30 mm	PS050130
32 mm	PS050132
34 mm	PS050134
36 mm	PS050136
38 mm	PS050138
40 mm	PS050140
42 mm	PS050142
44 mm	PS050144
46 mm	PS050146
48 mm	PS050148
50 mm	PS050150
55 mm	PS050155
60 mm	PS050160

PECA® Compressive specific instruments

Description	Reference
K-Wire Ø 1.4 lg 150 CrCo	CKW02005
Drill bit Ø3.2	XDB01018
Exact-T®10 screwdriver tip	XSD04004
Ruler lg 150	XGA01009
Nexis® / PECA®-C - countersink Ø 3.7*	XRE01007 *

* *Optional.*

Indications

Examples of post-operative X-Rays - MTP arthrodesis



Please Note:

Carefully read the enclosed Instructions For Use (IFU) and all packaging label information. Devices : Implants : Classe IIb-CE1639 / Instruments : Classe I / Classe IIa-CE1639.

Novastep:

2, Allée Jacques Frimot - 35000 RENNES - France
Tel : + 33 (0) 2 99 33 86 50 / Fax : + 33 (0) 9 70 29 18 95
contact@novastep-ortho.com / www.novastep-ortho.com

Reference: Nex-PECA-C-L-Ed3-11-22-EN