PECAPLASTY® TRAY OVERHEAD GUIDE

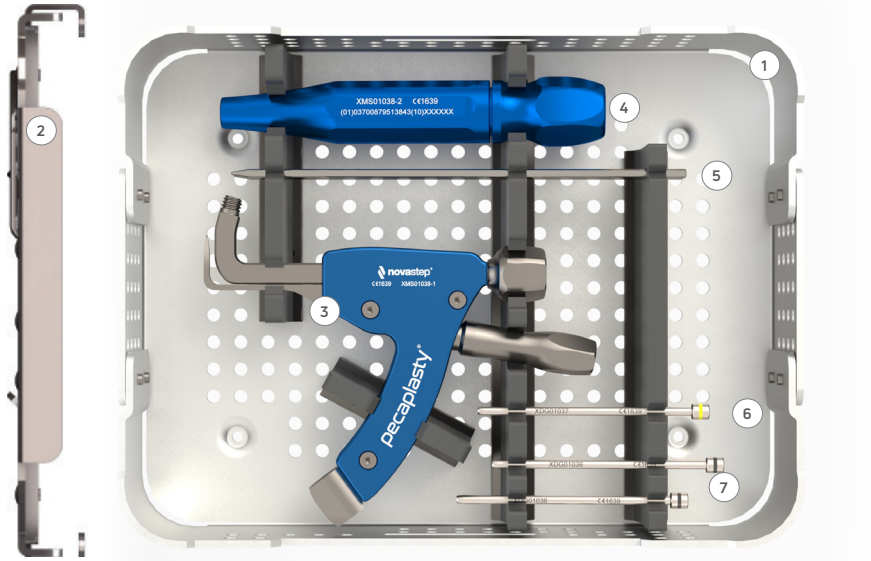

#	DESIGNATION	REFERENCE	QTY
1	TRAY	ACC1019P0001	1
2	LID	ACC1019P0002	1
3	TARGETING GUIDE	XMS01038-9	1
4	WIRE HANDLE FOR TARGETING GUIDE	XMS01038-2	1
5	TRACTION WIRE Ø2.5 LG 128 - STERILE[1][2]	SKW06002	5
6	PECA® Ø3 - K-WIRE SLEEVE	XDG01037	1
7	PECA® Ø4 - K-WIRE SLEEVE	XDG01036	2

[1] Sterile traction wire supplied separately

[2] Non sterile traction wire is also available (Ref: CKW06002)

T +33 (0) 2 99 33 86 50 F + 33 (0) 9 70 29 18 95

Legal manufacturer: Novastep® S.A.S
2 Allée Jacques Frimot | 35000 Rennes | France
contact-intfa@enovis.com
www.int.novastep.life
Copyright © 2024 Enovis Foot and Ankle

Carefully read the enclosed Instructions For Use (IFU) and all packaging label information. Devices: Implants: Class IIb-CE1639 / Instruments: Class I / Class Ir-CE1639 / Class IIa-CE1639.

REFERENCE: PECA-2.0-TAR-TL-ED9-07-26-EN